

## PRODUCT DATA SHEET


### Zepto™ Orange Carboxyl Microspheres

#### Description


Cytodiagnosics Zepto™ Fluorescent Carboxyl Microspheres are internally labeled with fluorophores synthesized using a unique proprietary protocol. Compared with solvent swelling or dye entrapment methods, our method produces microspheres with a greater range of fluorescence intensities (over several orders) and a greater number of available emission wavelengths, giving you as a customer more flexibility and choices in choosing a fluorescence profile. Our microspheres have wide working conditions and their fluorescence is less prone to environmental factors such as salt and heat with a longer shelf life.

Carboxyl surface functional groups are available for carbodiimide covalent conjugation of ligands, e.g. proteins, nucleic acids, and molecules with accessible primary amines. Such spheres are used extensively in cell tracking, fluidic tracing, biosensing, immunoassays, and imaging applications.

The excitation and emission spectra are illustrated in Figure 1. They are a suitable for flow cytometry-based assays. Their Forward Scatter (FSC) vs. Side Scatter (SSC) plot and fluorescence histogram in FL2 (488 nm excitation; 590 nm emission) on a typical flow cytometer are illustrated in Figure 2.



**Figure 1.** Excitation and emission spectra of Zepto™ Orange Carboxyl Microspheres.



**Figure 2.** FSC-SSC plot and fluorescence histogram in FL2 of Zepto™ Orange Carboxyl Microspheres on a flow cytometer.

#### Characteristics

Diameters:  $2.5 \pm 0.3 \mu\text{m}$   
 Concentration: 1E8/mL in ddH<sub>2</sub>O  
 Excitation max: 555 nm  
 Emission max: 570 nm  
 Surface Functional Group: -COOH  
 Carboxyl Parking Area:  $\sim 2.5 \text{ nm}^2/\text{-COOH group}$

#### Content

Zepto™ Orange Carboxyl Microspheres: supplied in 1 mL (Cat. #ZBC-5-1ML) or 5 mL (Cat. #ZBC-5-5ML) formats.

#### Storage/Stability

This product should be stored at 2-8°C. Avoid freezing, drying or prolonged exposure to light. For the best consistency and stability of microsphere fluorescence, the microspheres are best used in pH from 3 to 8, temperature up to 60 degrees, and salt concentration up to 0.5 M. Product is stable for at least 12 months when stored under the recommended conditions.

#### Usage Guidelines

*Covalent coupling of microspheres via carbodiimide coupling chemistry*

Zepto™ Orange Carboxyl Microspheres are designed for surface functionalization with molecules containing primary amines via carbodiimide crosslinkers such as 1-Ethyl-3-(3-dimethylaminopropyl)carbodiimide (EDC). Different molecules may require different conjugation



and detection assay conditions for optimal results. Researchers are advised to optimize parameters such as EDC and ligand concentrations (ratios), for their specific application, see page 3.

The following procedure provides general guidelines for conjugation of antibodies to Zepto™ Carboxyl Microspheres, and for their use in downstream assays. Multiple antibodies of different specificities, or other molecules of interest, may be conjugated to microspheres emitting different fluorescent colors, allowing for multiplexed detection capabilities in a single assay.

#### *Two-step conjugation procedure*

A typical conjugation reaction utilizes 10 million Zepto™ Carboxyl Microspheres. The following reagents are required and not provided with the product:

- Activation buffer: MES buffer (2-(N-morpholino)ethanesulfonic acid) 50 mM, pH 5.5
  - Washing buffer: 0.1X PBST (TWEEN20: 0.05% w/v)
  - Storage buffer: 1% bovine serum albumin in 0.1X PBST (Sigma, A3059), 0.09% sodium azide
  - EDC (Sigma E1769): 1 mg/mL in activation buffer, freshly prepared
  - IgG: 0.5 mg/mL in 0.5X PBS
1. Vortex the product bottle before using to ensure homogeneous suspension of the microspheres
  2. Immediately aliquot 10 million microspheres (100  $\mu$ L of stock solution as provided)
  3. Remove supernatant and add 500  $\mu$ L of EDC
  4. Mix well and activate for 30 min at room temperature
  5. Add 500  $\mu$ L of washing buffer and mix well
  6. Gently pellet at 500 g for 5 min \*
  7. Discard supernatant and add 50  $\mu$ L of IgG
  8. Mix well and incubate for 4 hours at room temperature with constant rotation
  9. Add 500  $\mu$ L of washing buffer and mix well
  10. Gently pellet at 500 g for 5 min
  11. Discard supernatant and add 500  $\mu$ L of washing buffer
  12. Gently pellet at 500 g for 5 min
  13. Discard supernatant and add 250  $\mu$ L of storage buffer and mix well
  14. Incubate for 1 hour at room temperature with rotation
  15. Conjugated microspheres are now ready for your use in assays. Alternatively, store at 4°C protected from light until use

\* *The centrifugation speed for pelleting microspheres is a range between 100 to 10,000 g. A lower/more gentle centrifugation speed with longer time is recommended to form a good microsphere pellet, especially after conjugation. Prolonged centrifugation at high speed may aggregate microspheres irreversibly.*


#### *Detection assay*

The following procedure is based on a sandwich assay for single analyte detection with flow cytometry. Capture antibodies are conjugated to the microsphere surface via EDC as described above. A reporter is typically a fluorophore-labeled antibody that recognizes and binds to a different domain or epitope on the analyte than that of the capture antibody. In the presence of analyte, a sandwich is formed when the microspheres coated with the capture antibody and the reporter antibody bind the analyte. The user may need to optimize assay parameters, or develop direct and multiplex assays for their specific application.

1. Aliquot 10  $\mu$ L of conjugated spheres as prepared above
2. Add 5  $\mu$ L of reporter antibody (50  $\mu$ g/mL in TBS, 0.1% BSA)
3. Add 100  $\mu$ L of analyte standard or sample solution and mix well
4. Incubate for 1 hour at room temperature with constant rotation
5. Add 500  $\mu$ L of washing buffer and mix well
6. Gently pellet at 500 g for 5 min
7. Discard supernatant, add 500  $\mu$ L of washing buffer and mix well
8. Gently pellet at 500 g for 5 min
9. Resuspend microspheres in washing buffer and analyze by flow cytometry

#### *Flow cytometry analysis*

1. Gate on the single population of microspheres on FSC vs. SSC plot (refer to Figure 2)
2. In the fluorescence channel for the reporter, the median values of fluorescence intensity for gated microsphere population determine the “negative” and “positive” by standards. Or the user defines the threshold value for positive detection

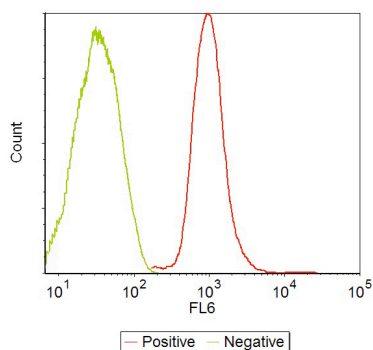

**Figure 3.** A typical protein detection assay using Zepto™ Carboxyl Microspheres on flow cytometry. The reporter is Cyto 633 dye detected in FL6 (635 nm excitation; 675 nm emission) of a flow cytometer. Histograms of “negative” (green) and “positive” (red) of the reporter fluorescence are shown above.

### Additional Information

#### *Optimizing the conjugation conditions*

The concentration ratio of microspheres to EDC and protein to the activated microspheres ratio may need to be optimized for optimal conjugation.

Sulfo-N-hydroxysuccinimide (NHS) can be added with EDC during activation to increase conjugation efficiency. NHS reacts with the o-acrylisourea intermediate formed by EDC and carboxyl group and replaces it with a more stable amine-reactive ester. The molecular ratio between EDC and NHS is typically at 1:1.

#### *Optimization of detection assay conditions*

The detection sensitivity is affected by various factors, such as conjugation efficiency, microsphere number and temperature of the detection assay. The user may need to titrate the amount of microspheres for the best sensitivity. For flow cytometry applications, the number of microspheres in gate ranges from 100 to 10000. Fewer microspheres generally leads to better sensitivity but also a higher variance of assays.

### Precautions and Disclaimer

These products are for R&D use only, not for drug, household, or other uses. Please consult the Material Safety Data Sheet available online at [www.cytodiagnosics.com](http://www.cytodiagnosics.com) for information regarding hazards and safe handling procedures.

### Ordering Information

For ordering call 866-344-3954 or visit us online at [www.cytodiagnosics.com](http://www.cytodiagnosics.com)